# BSL2 Aspirator Setup

In-line HEPA Filter

NO PHENOL
NO CHLOROFORM
NO ACETONE
NO XYLENE
NOTHING THAT
MELTS PLASTIC

Avoid direct aspiration through outlet!!

*outlet*

*outlet*

(F)     (B)     Vacuum source

HEPA

Primary Flask

Overflow Flask

*drierite*

Make sure its dated!

A

B

C

D
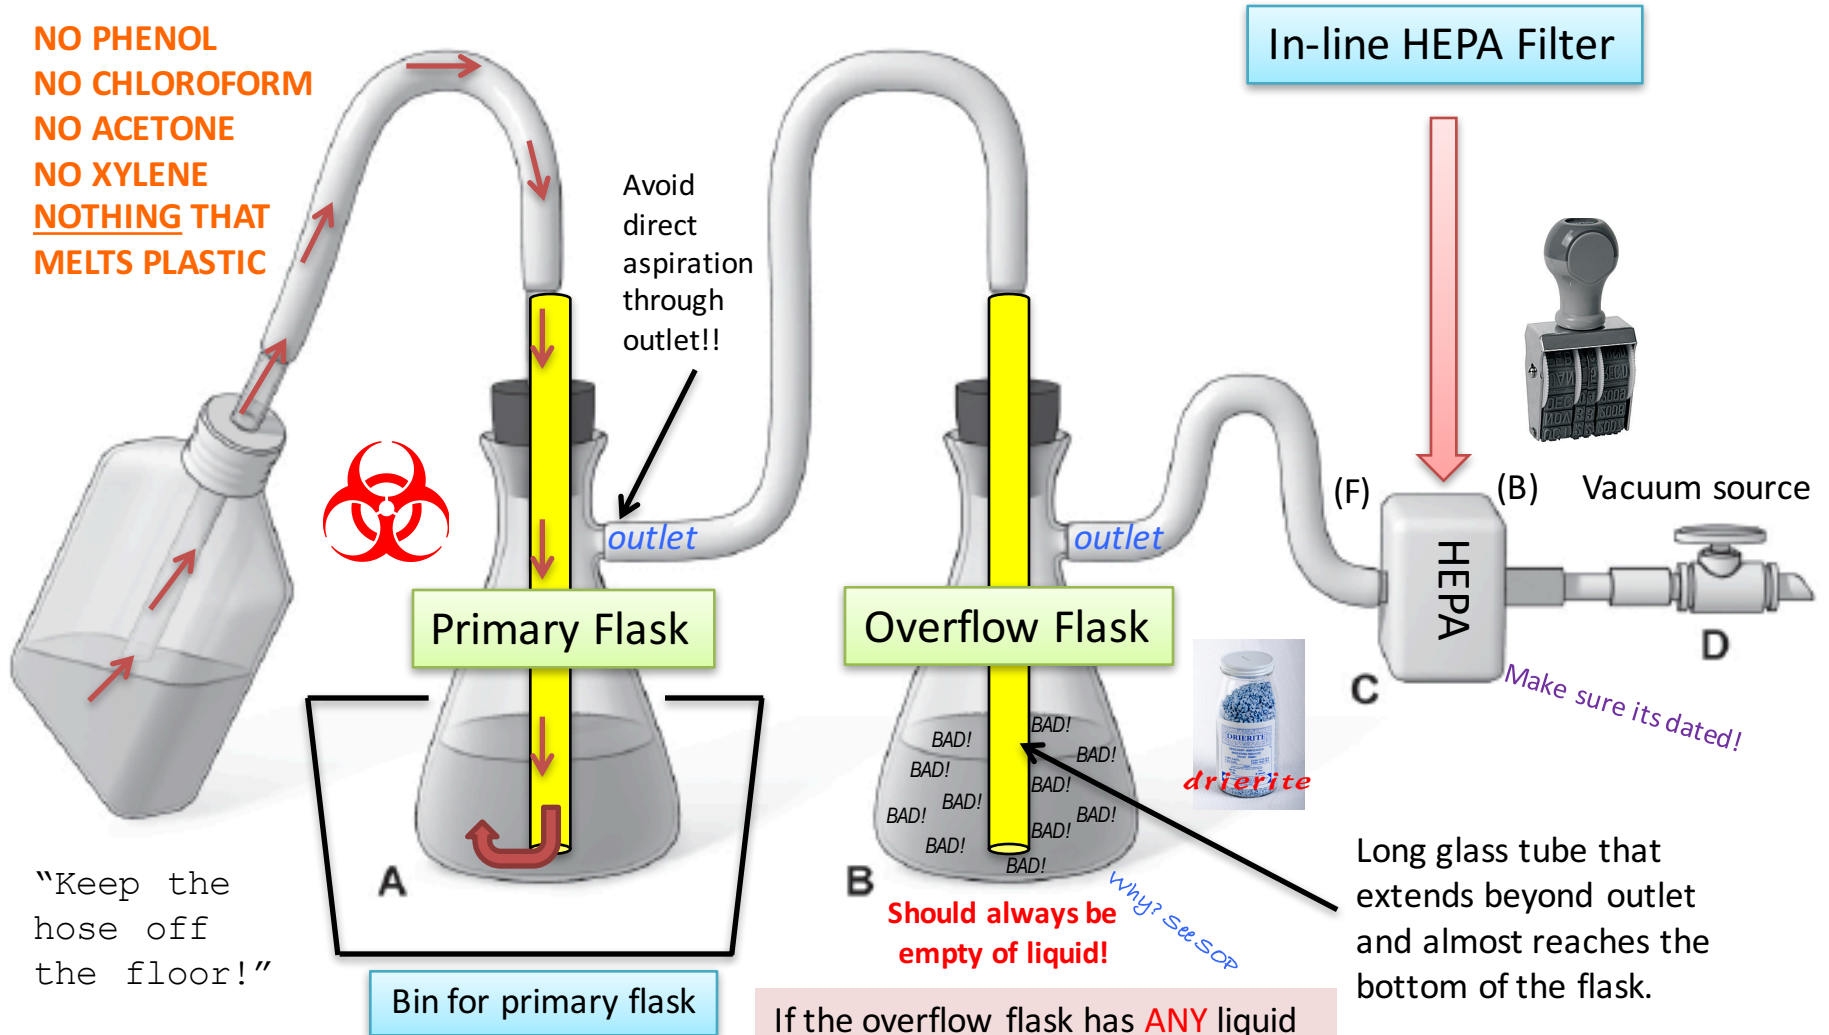
"Keep the hose off the floor!"

Should always be empty of liquid!

Why? See SOP

Long glass tube that extends beyond outlet and almost reaches the bottom of the flask.

Bin for primary flask

If the overflow flask has ANY liquid in it, disinfect, disassemble, clean and reassemble system.

BAD! BAD! BAD! BAD! BAD! BAD! BAD! BAD! BAD! BAD! BAD!

Created by
biosafety
@ McMaster

Base image from Biosafety in Microbiological and Biomedical Laboratories, CDC/NIH 5th Ed, 2009, p322